



Advanced flow cytometry

FASER Kit – PE

Order No. 130-091-764

Index

1. Description
 - 1.1 Background and product applications
 - 1.2 Reagent requirements
2. General protocol for immunofluorescent staining
3. Example of immunofluorescence amplification using the FASER Kit – PE

1. Description

Components	2×2 mL FcR Blocking Reagent, 1 mL PE-Activator (Reagent 1), 1 mL PE-Enhancer (Reagent 2).
Size	For 10 ⁹ total cells, up to 100 stainings.
Staining concentration	FcR Blocking Reagent is used at a dilution of 1:5. The PE-Activator (Reagent 1) and the PE-Enhancer (Reagent 2) are used at a dilution of 1:11.
Product format	Reagents are supplied as a solution containing 0.1% gelatine and 0.05% sodium azide.
Storage	Store protected from light at 4–8 °C. Do not freeze. The expiration date is indicated on the vial label.

1.1 Background and product applications

The FASER (Fluorescence Amplification by Sequential Employment of Reagents) Kit – PE (R-phycoerythrin) is developed to increase the fluorescence intensity of cells labeled with a PE-conjugated antibody. The intensity of the PE fluorescence is amplified by sequential addition of the PE-Activator (Reagent 1) and the PE-Enhancer (Reagent 2). For further enhancement of the fluorescence intensity, sequential addition of the PE-Activator (Reagent 1) and the PE-Enhancer (Reagent 2) can be repeated several times.

The FASER Kit – PE does not affect direct staining with other fluorochrome-conjugated antibodies, but should not be combined with indirect immunofluorescent staining using biotin-conjugated antibodies. The Kit is suitable for PE-labeled, fresh or formaldehyde-fixed cells of any type or species in suspension. Analysis is performed by flow cytometry.

Examples of product application

- Amplification of PE fluorescence which is weak, for example
 - due to PE-conjugated antibody staining of antigens which are expressed at low levels,
 - due to immunomagnetic and PE-conjugated antibody labeling of the same antigen epitope,
 - due to PE-conjugated antibody staining with a low affinity antibody.
- Amplification of the fluorescence signal of a PE-labeled cell fraction for a clearer flow cytometric discrimination from the non-labeled cell fraction.
- Amplification of magnetic labeling with Anti-PE MicroBeads (# 130-048-801) by increasing the number of Anti-PE MicroBead binding sites per cell.

1.2 Reagent requirements


- Buffer: PBS (phosphate buffered saline) pH 7.2, supplemented with 0.5% BSA (bovine serum albumin) and 2 mM EDTA. Keep buffer cold (4–8 °C).

▲ **Note:** EDTA can be replaced by other supplements such as anticoagulant citrate dextrose formula-A (ACD-A) or citrate phosphate dextrose (CPD). BSA can be replaced by other proteins such as serum albumin, serum or fetal calf serum. Buffers or media containing Ca²⁺ or Mg²⁺ are not recommended for use.

Antibody-labeled cell

1st Amplification round

2nd Amplification round

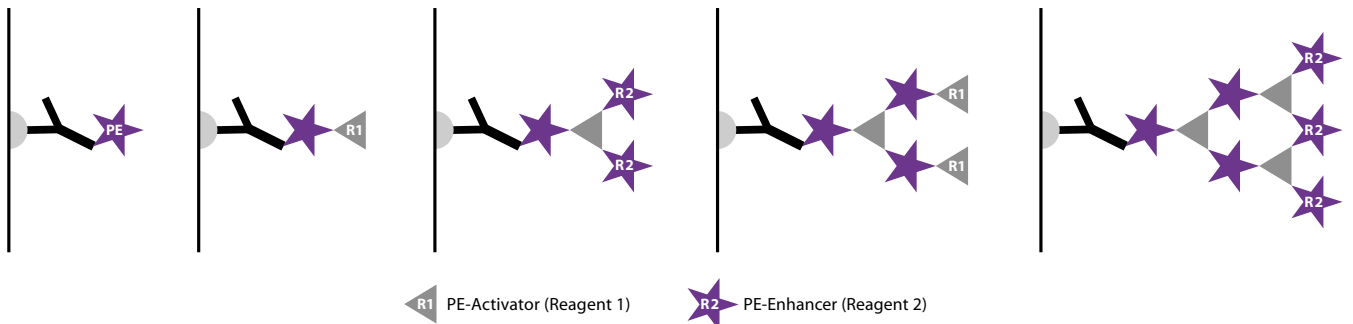

130-001-190/01

Miltenyi Biotec

www.miltenyibiotec.com



Miltenyi Biotec GmbH
Friedrich-Ebert-Str. 68
51429 Bergisch Gladbach, Germany
Phone +49-2204-8306-0 Fax +49-2204-85197

Miltenyi Biotec Inc.
12740 Earhart Avenue, Auburn CA 95602, USA
Phone 800 FOR MACS, 530 888-8871
Fax 530 888-8925

2. General protocol for immunofluorescent staining

▲ If formaldehyde fixation of cells is required, cells should be stained and treated with the FASER Kit – PE prior to fixation.

▲ If the FASER Kit – PE is used for amplification of magnetic labeling with Anti-PE MicroBeads, amplify PE staining as described below. For subsequent magnetic labeling, refer to the Anti-PE MicroBead data sheet.

▲ Volumes for fluorescent labeling given below are for up to 10^7 total cells. When working with fewer than 10^7 cells, use the same volumes as indicated. When working with higher cell numbers, scale up all reagent volumes and total volumes, accordingly (e.g. for 2×10^7 total cells, use twice the volume of all indicated reagent volumes and total volumes).

1. Label cells with desired PE-conjugated antibody and afterwards wash cells according to the manufacturer's recommendations.
2. Resuspend up to 10^7 cells in 80 μ L of buffer.
3. Add 20 μ L of **FcR Blocking Reagent**.
4. Add 10 μ L of **PE-Activator (Reagent 1)**.

5. Mix well and incubate for 10 minutes in the dark at 4–8 °C.


▲ **Note:** Working on ice requires increased incubation time. Higher temperatures and/or longer incubation times lead to non-specific cell labeling.

6. Wash cells by adding 1–2 mL of buffer per 10^7 cells and centrifuge at 300 \times g for 10 minutes. Pipette off supernatant completely.
7. Resuspend cell pellet in 80 μ L of buffer.
8. Add 20 μ L of **FcR Blocking Reagent**.
9. Add 10 μ L of **PE-Enhancer (Reagent 2)**.
10. Mix well and incubate for 10 minutes in the dark at 4–8 °C.

▲ **Note:** Working on ice requires increased incubation time. Higher temperatures and/or longer incubation times lead to non-specific cell labeling.
11. Wash cells by adding 1–2 mL of buffer per 10^7 cells and centrifuge at 300 \times g for 10 minutes. Pipette off supernatant completely.
12. (Optional) Repeat steps 2–11, if further amplification of the PE fluorescence is required.
13. Finally resuspend cell pellet in a suitable amount of buffer for analysis by flow cytometry.

3. Example of immunofluorescence amplification using the FASER Kit – PE

Human peripheral blood mononuclear cells (PBMC) were stained with CD19-PE, human (# 130-091-247), and the PE fluorescence was increased by two rounds of amplification using the FASER Kit – PE. Cells were analyzed by flow cytometry. Cell debris and dead cells were excluded from the analysis based on scatter signals and propidium iodide (PI) fluorescence.

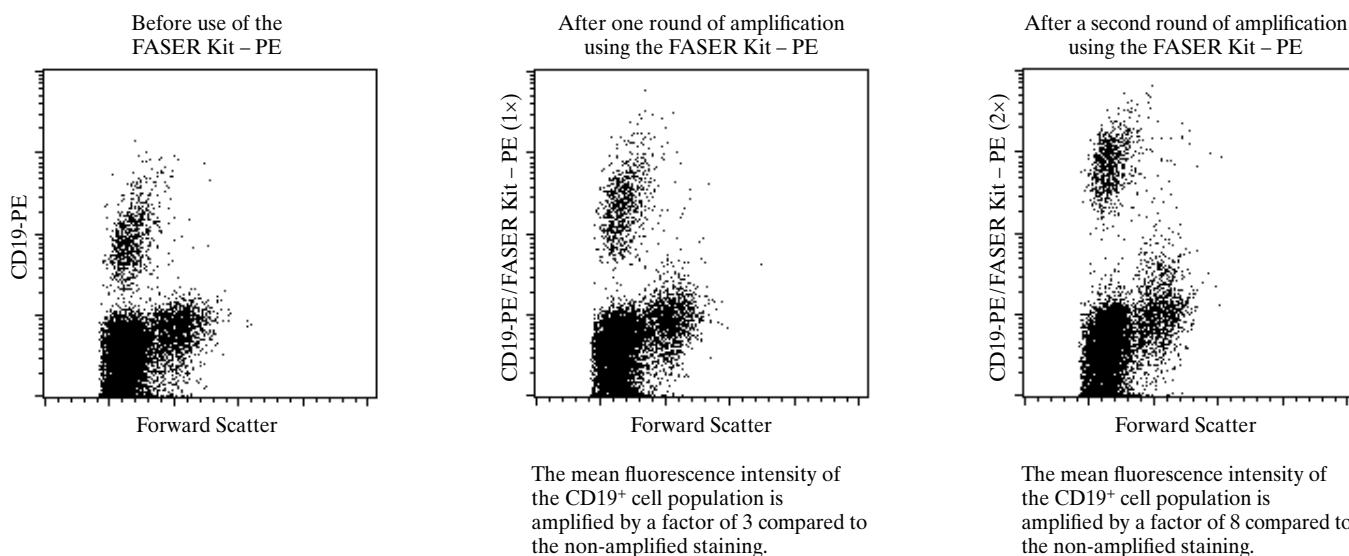

Warning

Reagents contain sodium azide. Sodium azide yields hydrazoic acid under acid conditions, which is extremely toxic. Azide compounds should be diluted with running water before discarded. These precautions are recommended to avoid deposits in plumbing where explosive conditions may develop.

Warranty

The products sold hereunder are warranted only to be free from defects in workmanship and material at the time of delivery to the customer. MILTENYI BIOTECH GmbH makes no warranty or representation, either expressed or

implied, with respect to the suitability of a product for a particular purpose. There are no warranties, expressed or implied, which extend beyond the Technical Specifications of the products. MILTENYI BIOTECH GmbH's liability is limited to either replacement of the products or refund of the purchase price.

MILTENYI BIOTECH GmbH is not liable for any property damage, personal injury or economic loss caused by the product.

MACS® is a registered trademark of Miltenyi Biotec GmbH.